


Pyrolysis-GC/MS to Characterize Indoor Dust

As indoor dust may contain toxic materials along with allergen causing natural polymers from spiders, insects and mites, the study of indoor dust can be used to determine potential environmental health risks in the environment. Using a CDS Pyroprobe as an injection strategy for gas chromatography/mass spectrometry, we are able to understand both the semi-volatile and polymer nature of dust.

We took dust from kitchens, bathrooms, and bedrooms in homes, and ran them on the GC/MS using a CDS Pyroprobe 5200 to introduce the samples. Small amounts of dust (<100µg) were desorbed at 300°C, and then pyrolyzed at 750°C. As expected, dust collected turned out to be a complex mixture. In this study, just a few components were identified. Each location had pyrolysis products such as phenols from wool and hair, levoglucosan and furans from cellulose (cotton or paper), benzoic acid from polyester (clothing and carpeting), and styrene from polystyrene. Furthermore, not all locations were identical; each contained different types and relative amounts of products, relating to the items found in the area. For example, home “K”, furnished with polyester carpeting, had more polyester; and home “T” had more cellulose from cotton clothing.

Semivolatiles present included fatty acids and cholesterol from skin and cooking oils, and the plasticizer bis(2-ethylhexyl) phthalate. By sampling dust, and items suspected of contributing to dust, thermal desorption and pyrolysis GC/MS can be used to help identify dust make-up.

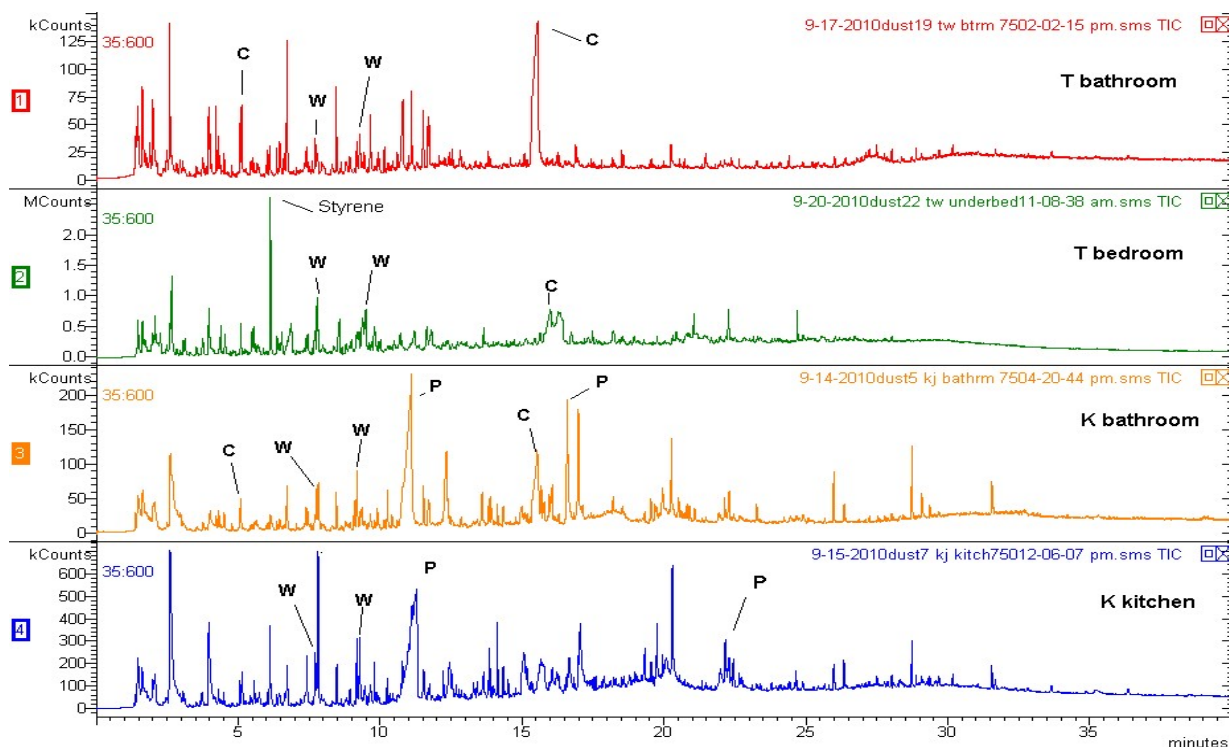

Peaks from Wool or Hair(W), Cotton (C), and Polyester (P) labeled in four dust samples.

Equipment

CDS Model 5200 Pyroprobe in direct (no trapping) mode interfaced to a Varian 3800 GC Saturn 2000 Ion Trap detector.

Model 5200 Conditions

Desorption:

Valve Oven: 325°C

Transfer Line: 325°C

Pyroprobe Temperature: 300°C

Pyroprobe Time: 15 seconds

Interface Final: 300°C for 3 minutes

Pyrolysis:

Valve Oven: 325°C

Transfer Line: 325°C

Pyroprobe Temperature: 750°C

Pyroprobe Time: 15 seconds

Interface Final: 325°C for 3 minutes

GC Conditions

Carrier: Helium

Injector: 325°C

Split: 50:1

Column: 5% phenyl (30m X 0.25mm)

Detector: Ion Trap

Range: 35 - 550amu

GC Program:

Initial: 40°C for 2 minutes

Ramp: 10°C/min.

Final: 300°C for 5 minutes

FOR MORE INFORMATION
CONCERNING THIS APPLICATION,
WE RECOMMEND THE
FOLLOWING READING:

K. Jansson et. al., Multistep thermal characterization of polymers using GC-MS, American Lab, 39 (6) (2007) 16-19.

© courtesy of CDS Analytical Inc.

Headquarters

JSB International
Tramstraat 15
5611 CM Eindhoven
T +31 (0) 40 251 47 53
F +31 (0) 40 251 47 58

Zoex Europe
Tramstraat 15
5611 CM Eindhoven
T +31 (0) 40 257 39 72
F +31 (0) 40 251 47 58

Sales and Service

Netherlands
Apolloweg 2B
8239 DA Lelystad
T +31 (0) 320 87 00 18
F +31 (0) 320 87 00 19

Belgium
Grensstraat 7
Box 3 1831 Diegem
T +32 (0) 2 721 92 11
F +32 (0) 2 720 76 22

Germany
Max-Planck-Strasse 4
D-47475 Kamp-Lintfort
T +49 (0) 28 42 9280 799
F +49 (0) 28 42 9732 638

UK & Ireland
Cedar Court,
Grove Park Business Est.
White Waltham, Maidenhead
Berks, SL6 3LW
T +44 (0) 16 288 220 48
F +44 (0) 70 394 006 78

info@go-jsb.com
www.go-jsb.com

